

Myostatin (MSTN) CLIA Kit | MSTN clia kit

CLIA Kit for Myostatin (MSTN)

CATALOG #
AAA130519


PRODUCT SYNONYMS

Myostatin (MSTN); CLIA Kit for Myostatin (MSTN); MSTN clia kit

PRODUCT SPECIFICATIONS

Specificity	This assay has high sensitivity and excellent specificity for detection of Myostatin (MSTN) No significant cross-reactivity or interference between Myostatin (MSTN) and analogues was observed.
Sequence Length	459
Assay Type	Sandwich
Samples	Serum, plasma and other biological fluids
Detection Range	6.859-5000pg/mL The standard curve concentrations used for the ELISA's were 5000pg/mL, 1666.67pg/mL, 555.56pg/mL, 185.19pg/mL, 61.728pg/mL, 20.576pg/mL, 6.859pg/mL
Sensitivity	The minimum detectable dose of this kit is typically less than 19pg/mL
Precision	Intra-assay Precision (Precision within an assay): 3 samples with low, middle and high level Myostatin (MSTN) were tested 20 times on one plate, respectively. Inter-assay Precision (Precision between assays): 3 samples with low, middle and high level Myostatin (MSTN) were tested on 3 different plates, 8 replicates in each plate. $CV(\%) = SD/mean \times 100$ Intra-Assay: $CV < 10\%$ Inter-Assay: $CV < 12\%$
Organism Species	Mus musculus (Mouse)
Assay Length	4.5 hours
Preparation and Storage	The stability of kit is determined by the loss rate of activity. The loss rate of this kit is less than 5% within the expiration date under appropriate storage condition. To minimize extra influence on the performance, operation procedures and lab conditions, especially room temperature, air humidity, incubator temperature should be strictly controlled. It is also strongly suggested that the whole assay is performed by the same operator from the beginning to the end.

IMAGES

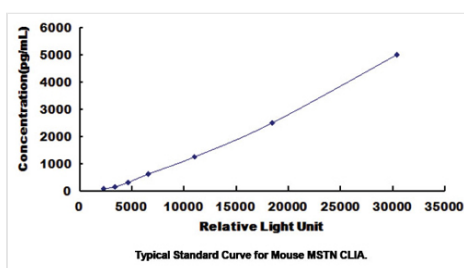

Standard Curve (Sample)

ADDITIONAL INFORMATION

Related Product Information for MSTN clia kit	The microtiter plate provided in this kit has been pre-coated with an antigen. Standards or samples are then added to the appropriate microtiter plate wells with a biotin-conjugated secondary antibody. Next, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. Then the mixture of substrate A and B is added to generate glow light emission kinetics. Upon plate development, the intensity of the emitted light is proportional to the Myostatin (MSTN) level in the sample or standard.
---	--

NCBI AND UNIPROT INFORMATION

NCBI GI #	308445232
NCBI Official Full Name	myostatin

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Small volumes of product may become entrapped in the seal of the vial during shipment and storage; if necessary, briefly centrifuge the vial on a tabletop centrifuge to dislodge any liquid in the cap.

AAA Biotech | Tel: +1 (619) 604-9440 | Fax: +1 (619) 604-9441 | contact@aaabiotech.com
Online datasheet: <https://stage.aaabiotech.com/clia-kits/myostatin-mstn/130519>