

Human DAO (Diamine Oxidase) CLIA Kit | DAO clia kit

Human DAO (Diamine Oxidase) CLIA Kit

CATALOG #
AAA171003

REACTIVITY
Human


PRODUCT SYNONYMS

DAO (Diamine Oxidase); Human DAO (Diamine Oxidase) CLIA Kit; AOC1; ABP1; Amiloride Binding Protein 1; Amine Oxidase (Copper-Containing); DAO clia kit

PRODUCT SPECIFICATIONS

Reactivity	Human
Specificity	This kit recognizes natural and recombinant DAO. No significant cross-reactivity or interference between DAO and analogues was observed.
Sequence Length	675
Assay Type	Sandwich
Detection Range	0.781-50ng/mL
Sensitivity	Min: 0.469ng/mL; Max: 50ng/mL

IMAGES

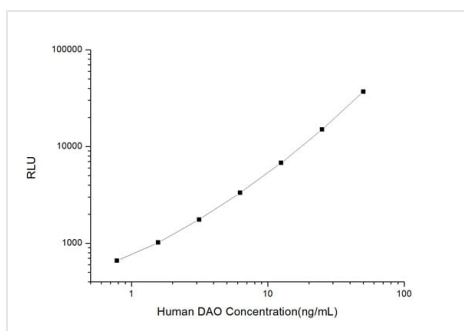

Standard Curve (Sample)

ADDITIONAL INFORMATION

Related Product Information for DAO clia kit

Intended Uses: This CLIA kit applies to the in vitro quantitative determination of DAO concentrations in serum, plasma and other biological fluids.

Principle of the Assay: This kit uses Sandwich-CLIA as the method. The micro CLIA plate provided in this kit has been pre-coated with an antibody specific to DAO. Standards or samples are added to the appropriate micro CLIA plate wells and combined with the specific antibody. Then a biotinylated detection antibody specific for DAO and Avidin-Horseradish Peroxidase (HRP) conjugate is added to each micro plate well successively and incubated. Free components are washed away. The substrate solution is added to each well. Only those wells that contain DAO, biotinylated detection antibody and Avidin-HRP conjugate will appear fluorescence. The Relative light unit (RLU) value is measured spectrophotometrically by the Chemiluminescence immunoassay analyzer. The RLU value is positively associated with the concentration of DAO. You can calculate the concentration of DAO in the samples by comparing the RLU value of the samples to the standard curve.

NCBI AND UNIPROT INFORMATION

NCBI GI #	430769122
Molecular Weight	76,297 Da
NCBI Official Full Name	diamine oxidase
UniProt Protein Name	Amine oxidase
UniProt Entry Name	A0A059PAW8_VICFA

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Small volumes of product may become entrapped in the seal of the vial during shipment and storage; if necessary, briefly centrifuge the vial on a tabletop centrifuge to dislodge any liquid in the cap.

AAA Biotech | Tel: +1 (619) 604-9440 | Fax: +1 (619) 604-9441 | contact@aaabiotech.com
Online datasheet: <https://stage.aaabiotech.com/human-clia-kits/dao-diamine-oxidase/171003>