

Mouse Matrix Metalloproteinase 1 (MMP1) CLIA Kit | MMP1 clia kit

Mouse Matrix Metalloproteinase 1 (MMP1) CLIA Kit

CATALOG # AAA188846	REACTIVITY Mouse	APPLICATIONS CLIA (Chemiluminescence Immunoassay)
-------------------------------	----------------------------	---


PRODUCT SYNONYMS

Matrix Metalloproteinase 1 (MMP1); Mouse Matrix Metalloproteinase 1 (MMP1) CLIA Kit; Matrix Metalloproteinase 1; CLGN; CLG1; Collagenase; Interstitial Collagenase; Vertebrate Collagenase; Fibroblast Collagenase; MMP1 clia kit

PRODUCT SPECIFICATIONS

Reactivity	Mouse
Specificity	This assay has high sensitivity and excellent specificity for detection of Matrix Metalloproteinase 1 (MMP1). No significant cross-reactivity or interference between Matrix Metalloproteinase 1 (MMP1) and analogues was observed.
Sequence Length	464
Assay Type	Double-antibody Sandwich
Samples	Serum, plasma, tissue homogenates, cell lysates, cell culture supernates and other biological fluids
Detection Range	27.4-20,000pg/mL
Sensitivity	The minimum detectable dose of this kit is typically less than 9.7pg/mL
Applicable Applications for MMP1 clia kit	CLIA (Chemiluminescence Immunoassay)
Precision	Intra-assay Precision (Precision within an assay): 3 samples with low, middle and high level Matrix Metalloproteinase 1 (MMP1) were tested 20 times on one plate, respectively. Inter-assay Precision (Precision between assays): 3 samples with low, middle and high level Matrix Metalloproteinase 1 (MMP1) were tested on 3 different plates, 8 replicates in each plate. $CV(\%) = SD/mean \times 100$ Intra-Assay: CV<10% Inter-Assay: CV<12%
Test Principle	The microplate provided in this kit has been pre-coated with an antibody specific to Matrix Metalloproteinase 1 (MMP1). Standards or samples are then added to the appropriate microplate wells with a biotin-conjugated antibody specific to Matrix Metalloproteinase 1 (MMP1). Next, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. Then the mixture of substrate A and B is added to generate glow light emission kinetics. Upon plate development, the intensity of the emitted light is proportional to the Matrix Metalloproteinase 1 (MMP1) level in the sample or standard.
Preparation and Storage	The stability of kit is determined by the loss rate of activity. The loss rate of this kit is less than 5% within the expiration date under appropriate storage condition. To minimize extra influence on the performance, operation procedures and lab conditions, especially room temperature, air humidity, incubator temperature should be strictly controlled. It is also strongly suggested that the whole assay is performed by the same operator from the beginning to the end.

IMAGES

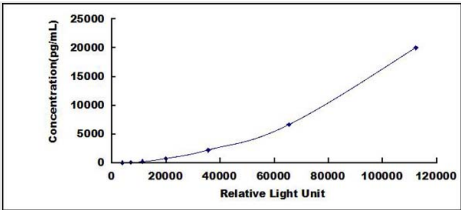

Standard Curve (Sample)

NCBI AND UNIPROT INFORMATION

NCBI GI #	14030785
NCBI GeneID	83995
NCBI Accession #	NP_114395.1
NCBI GenBank Nucleotide #	NP_114395.1
UniProt Accession #	Q9EPL5
NCBI Official Full Name	interstitial collagenase A preproprotein
NCBI Official Synonym Full Names	matrix metalloproteinase 1a (interstitial collagenase)
NCBI Official Symbol	Mmp1a
NCBI Official Synonym Symbols	Mcola; MMP-1a; Mcol-A
NCBI Protein Information	interstitial collagenase A
UniProt Protein Name	Interstitial collagenase A
UniProt Gene Name	Mmp1a
UniProt Synonym Gene Names	McolA; MMP-1a
UniProt Entry Name	MMP1A_MOUSE

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Small volumes of product may become entrapped in the seal of the vial during shipment and storage; if necessary, briefly centrifuge the vial on a tabletop centrifuge to dislodge any liquid in the cap.

AAA Biotech | Tel: +1 (619) 604-9440 | Fax: +1 (619) 604-9441 | contact@aaabiotech.com
Online datasheet: <https://stage.aaabiotech.com/mouse-clia-kits/matrix-metalloproteinase-1-mmp1/188846>