

Human Hyaluronidase (HAase) CLIA Kit | HAase clia kit

Human Hyaluronidase (HAase) CLIA Kit

CATALOG # AAA189012	REACTIVITY Human	APPLICATIONS CLIA (Chemiluminescence Immunoassay)
-------------------------------	----------------------------	---


PRODUCT SYNONYMS

Hyaluronidase (HAase); Human Hyaluronidase (HAase) CLIA Kit; Hyaluronidase; Hyaluronic Lase; Hyaluronidase; HAase clia kit

PRODUCT SPECIFICATIONS

Reactivity	Human
Specificity	This assay has high sensitivity and excellent specificity for detection of Hyaluronidase (HAase). No significant cross-reactivity or interference between Hyaluronidase (HAase) and analogues was observed.
Sequence Length	435
Assay Type	Double-antibody Sandwich
Samples	Serum, plasma, tissue homogenates and other biological fluids
Detection Range	0.69-500ng/mL
Sensitivity	The minimum detectable dose of this kit is typically less than 0.28ng/mL
Applicable Applications for HAase clia kit	CLIA (Chemiluminescence Immunoassay)
Precision	Intra-assay Precision (Precision within an assay): 3 samples with low, middle and high level Hyaluronidase (HAase) were tested 20 times on one plate, respectively. Inter-assay Precision (Precision between assays): 3 samples with low, middle and high level Hyaluronidase (HAase) were tested on 3 different plates, 8 replicates in each plate. CV(%) = SD/meanX100 Intra-Assay: CV<10% Inter-Assay: CV<12%
Test Principle	The microplate provided in this kit has been pre-coated with an antibody specific to Hyaluronidase (HAase). Standards or samples are then added to the appropriate microplate wells with a biotin-conjugated antibody specific to Hyaluronidase (HAase). Next, Avidin conjugated to Horseradish Peroxidase (HRP) is added to each microplate well and incubated. Then the mixture of substrate A and B is added to generate glow light emission kinetics. Upon plate development, the intensity of the emitted light is proportional to the Hyaluronidase (HAase) level in the sample or standard.
Preparation and Storage	The stability of kit is determined by the loss rate of activity. The loss rate of this kit is less than 5% within the expiration date under appropriate storage condition. To minimize extra influence on the performance, operation procedures and lab conditions, especially room temperature, air humidity, incubator temperature should be strictly controlled. It is also strongly suggested that the whole assay is performed by the same operator from the beginning to the end.

IMAGES

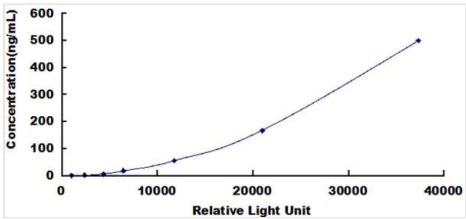

Standard Curve (Sample)

NCBI AND UNIPROT INFORMATION

NCBI GI #	74735617
NCBI GeneID	3373
UniProt Accession #	Q12794
NCBI Official Full Name	Hyaluronidase-1
NCBI Official Synonym Full Names	hyaluronidase 1
NCBI Official Symbol	HYAL1
NCBI Official Synonym Symbols	MPS9; NAT6; LUCA1; HYAL-1
NCBI Protein Information	hyaluronidase-1
UniProt Protein Name	Hyaluronidase-1
UniProt Gene Name	HYAL1
UniProt Synonym Gene Names	LUCA1; Hyal-1; LuCa-1
UniProt Entry Name	HYAL1_HUMAN

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Small volumes of product may become entrapped in the seal of the vial during shipment and storage; if necessary, briefly centrifuge the vial on a tabletop centrifuge to dislodge any liquid in the cap.

AAA Biotech | Tel: +1 (619) 604-9440 | Fax: +1 (619) 604-9441 | contact@aaabiotech.com
Online datasheet: <https://stage.aaabiotech.com/human-clia-kits/hyaluronidase-haase/189012>