

Canine Thyroid stimulating immunoglobulin ELISA Kit | TSI elisa kit

Canine Thyroid stimulating immunoglobulin ELISA Kit

CATALOG #
AAA89360

REACTIVITY
Canine


PRODUCT SYNONYMS

Thyroid stimulating immunoglobulin; Canine Thyroid stimulating immunoglobulin ELISA Kit; TSI elisa kit

PRODUCT SPECIFICATIONS

Reactivity	Canine
Samples	Serum, plasma, Cell Culture Supernatants, body fluid and tissue homogenate
Assay Type	Sandwich
Detection Range	2.5-50u/mL
Sensitivity	1.0 u/mL
Intended Uses	This TSI ELISA kit is a 1.5 hour solid-phase ELISA designed for the quantitative determination of Canine TSI. This ELISA kit for research use only, not for therapeutic applications!
Preparation and Storage	Store all reagents at 2-8 degree C.

IMAGES

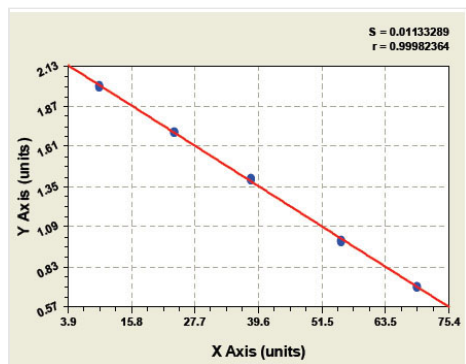

Standard Curve (Sample)

ADDITIONAL INFORMATION

Related Product Information for TSI elisa kit

Principle of the Assay: TSI ELISA kit applies the competitive enzyme immunoassay technique utilizing a monoclonal anti-TSI antibody and an TSI-HRP conjugate. The assay sample and buffer are incubated together with TSI-HRP conjugate in pre-coated plate for one hour. After the incubation period, the wells are decanted and washed five times. The wells are then incubated with a substrate for HRP enzyme. The product of the enzyme-substrate reaction forms a blue colored complex. Finally, a stop solution is added to stop the reaction, which will then turn the solution yellow. The intensity of color is measured spectrophotometrically at 450nm in a microplate reader. The intensity of the color is inversely proportional to the TSI concentration since TSI from samples and TSI-HRP conjugate compete for the anti-TSI antibody binding site. Since the number of sites is limited, as more sites are occupied by TSI from the sample, fewer sites are left to bind TSI-HRP conjugate. A standard curve is plotted relating the intensity of the color (O.D.) to the concentration of standards. The TSI concentration in each sample is interpolated from this standard curve.

For Research Use Only. Not for use in diagnostic or therapeutic procedures. Small volumes of product may become entrapped in the seal of the vial during shipment and storage; if necessary, briefly centrifuge the vial on a tabletop centrifuge to dislodge any liquid in the cap.

AAA Biotech | Tel: +1 (619) 604-9440 | Fax: +1 (619) 604-9441 | contact@aaabiotech.com

Online datasheet: <https://stage.aaabiotech.com/tsi-canine-elisa-kits/thyroid-stimulating-immunoglobulin/89360>